




EM-Tec B100 Faraday cup for beam current measurements

[Product # 36-000800](#)

Introduction

Precise beam current measurements are needed to check the stability of the electron or ion beam over longer periods of time or to adjust to a specific beam current. This might be needed for:

- quantitative X-ray micro-analysis when using references standards
- uniform and reproducible X-ray mappings and line scan
- electron beam lithography
- comparative measurements
- adjusting ion beam milling rates.

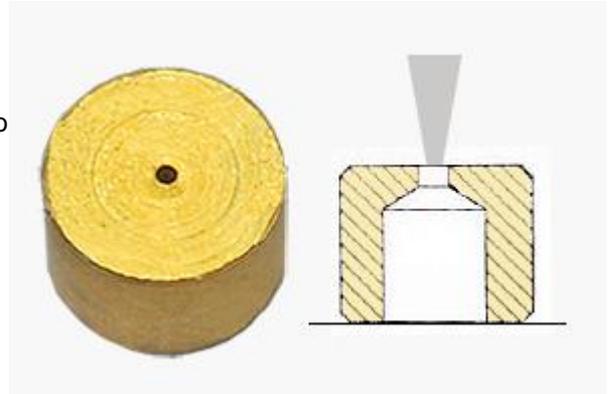

Measuring the beam current at the point where the beam hits the sample surface gives the most accurate results. A Faraday cup is a useful tool for precise measurements of the electron or ion beam. It consists of an enclosed cavity with a small opening through which the beam can be directed.

Sometimes beam measurements are made on graphite (carbon) or an electron beam aperture glued with carbon cement is used. Both methods are less precise:

- measuring beam current on carbon will not account for backscattered and secondary electrons
- an aperture glued with carbon cement lacks a larger cavity; it is only precise when underneath the aperture a larger cavity has been constructed.

EM-Tec B100 Faraday cup construction

The [EM-Tec B100](#) consists of single piece of brass with outside dimensions of $\varnothing 2.5 \times 2$ mm. The top of the Faraday cup includes a $\varnothing 100\mu\text{m}$ hole. Behind this $100\mu\text{m}$ aperture, there is a larger cavity of approximately $\varnothing 1.4 \times 1.5$ mm. When used, the EM-Tec B100 Faraday cup must be mounted on a sample stub or sample holder with conductive carbon cement and the small $\varnothing 100\mu\text{m}$ aperture facing the pole piece of the SEM.

When the electron or ion beam is directed into the middle of the small aperture; all primary, backscattered and virtually all secondary electrons are absorbed by the Faraday cup and hence the beam current can be determined. When properly used, the EM-Tec B100 Faraday cup efficiency is $>99\%$ in the 2-30kV range.

Specifications of the EM-Tec B100 Faraday cup:

Product #	#36-000800
Material	Brass
Outside Diameter	$\varnothing 2.5$ mm
Height	2mm
Hole size	$\varnothing 100\mu\text{m}$
Cavity size	$\varnothing 1.4 \times 1.5$ mm



Directions for using the EM-Tec B100 Faraday cup

When using the [EM-Tec B100 Faraday cup](#) on your SEM, FESEM, FIB or Microprobe system, the holder with the Faraday cup must be electrically connected to the sample stage. Select point mode on your system and make sure that the beam is directed in the middle of the aperture of the Faraday cup. If your system includes an absorbed current meter you can use this meter to measure the beam current.

If your system does not include an absorbed current meter, you have to connect a pico-ammeter (range 10^{-3} to 10^{-12} A) using a ground connection on the outside of the SEM chamber. Most SEMs provide such a connection on the outside of the SEM chamber or on the SEM chamber door. This is most likely a BNC connector capped with a metal cap to ensure proper grounding. Removal of the metal cap and connecting the pico-ammeter enables measuring the beam current. The power to the pico-ammeter needs to be provided by the same electrical circuit as the SEM. When removing the pico-ammeter, re-install the metal cap on the connector.

If the grounding cable from the SEM sample stage is connected to the inside of the SEM chamber, please consult the manufacturer or your service engineer if they can provide an absorbed current feedthrough.

With the measurement circuit installed, mount the EM-Tec B100 Faraday cup on the SEM sample stage and position the Faraday cup under the beam. Use point mode (or very high magnification scanning mode) to direct the beam into the middle of the aperture of the Faraday cup. Adjust condenser settings to change or require the desired beam current, note the beam current.

Maintenance, handling and cleaning

Store the [EM-Tec B100 Faraday cage](#) in a dust free and clean environment. Remove dust for use with a blower or duster.

Handle the EM-Tec B100 Faraday cup with plastic tweezers or plastic tipped tweezers to avoid damage of the relatively soft brass.

When used under normal conditions there is no maintenance or cleaning needed. If the aperture opening gets contaminated or charging occurs, the aperture opening needs to be cleaned:

- either use a plasma cleaner to remove carbon deposits
- or use mechanical cleaning with Wenol metal polish (#53-000100) or diamond polishing paste (29-001599) and wooden picks (#52-005023). Sonicate afterward in a 50/50 solution of isopropanol/acetone and let dry. If solvents are used, remounting with conductive carbon cement will be necessary

TSB 36-000800 EM-Tec B100 Faraday cup 2022-04-15 Revision 2